



Sartopore® 2 XLI 0.2 µm

Sterilizing Grade Filter Cartridges



Specifications

Materials

Prefilter Membrane:	PES, asymmetric
Endfilter Membrane:	PES, asymmetric
Support Fleece:	Polypropylene
Core:	Polypropylene
End Caps:	Polypropylene
O-Rings:	Silicone

Pore Size Combination

0.35 µm + 0.2 µm

Available Sizes | Filtration Area

Size 1	10"	0.8 m ² 8.6 ft ²
Size 2	20"	1.6 m ² 17.2 ft ²
Size 3	30"	2.4 m ² 25.8 ft ²

Available Adapters

25

Operating Parameters

Max. Allowable	5 bar 72.5 psi at 20°C
Differential Pressure:	2 bar 29 psi at 80°C
Max. Allowable Back Pressure:	2 bar 29 psi at 20°C

Description

Sartopore® 2 XLI filter cartridges are especially designed for sterilizing grade filtration of pharmaceutical solutions with a homogenous particle spectrum. The unique heterogeneous double layer PES membrane combination of Sartopore® 2 XLI cartridges is specifically developed to provide exceptional high total throughputs and outstanding flow rates for totally chemically defined process fluids and other process fluids of biotech manufacturing processes with small particle spectrum.

Applications

Typical applications of Sartopore® 2 XLI cartridges include sterilizing grade filtration of:

- Ophthalmic solutions
- Chemically defined cell culture media
- High viscous large volume parenterals
- Any fully chemically defined media

Economy

The combination of the build in 0.35 µm pre-filter in front of a 0.2 µm final filter together with an exceptionally high effective filtration area of 0.8 m²/10" cartridge provide outstanding total throughput and flow rate performance in the target applications. Thus ensuring highest process efficiency, minimized filtration costs and short filtration cycle times.

Compatibility

The PES membrane of Sartopore® 2 XLI cartridges provides broad chemical compatibility from pH 1 to pH 14 and low extractable levels. They are compatible with multiple in line steam sterilization cycles up to 134°C.

Scalability

Sartopore® 2 XLI filter elements are available in a broad range of sizes and formats to provide linear scale-up from R&D to process scale.

Microbiological Retention

Sartopore® 2 XLI filter cartridges are fully validated as sterilizing grade filters according to HIMA and ASTM F-838-05 guidelines.

Quality Control

Each individual element is tested for integrity by B.-P. and Diffusion-Test prior to be released assuring absolute reliability.

Documentation

Sartopore® 2 XLI cartridges are designed, developed and manufactured in accordance with an ISO 9001 certified Quality Management System. A Validation Guide is available for compliance with regulatory requirements.

По вопросам продаж и поддержки обращайтесь:

Астана+7(7172)727-132, Волгоград(844)278-03-48, Воронеж(473)204-51-73, Екатеринбург(343)384-55-89,
Казань(843)206-01-48, Краснодар(861)203-40-90, Красноярск(391)204-63-61, Москва(495)268-04-70,
Нижний Новгород(831)429-08-12, Новосибирск(383)227-86-73, Ростов-на-Дону(863)308-18-15, Самара(846)206-03-16,
Санкт-Петербург(812)309-46-40, Саратов(845)249-38-78, Уфа(347)229-48-12

sst@nt-rt.ru || sartorius.nt-rt.ru

Specifications

Extractables

Sartopore® 2 XLI 0.2 µm rated filter cartridges meet, or exceed the requirements for WFI quality standards set by the current USP.

Regulatory Compliance

Individually integrity tested

Integrity test correlated to HIMA/ASTM F 838-05 Bacteria Challenge Test

Non pyrogenic according to USP Bacterial Endotoxins

Pass USP Plastic Class VI Test

Non fiber releasing according to 21 CFR

Sterilization

In-Line Steam Sterilization:

134°C, 20 min. at max differential pressure of 0.5 bar

Autoclaving:

134°C, 2 bar, 30 min

Sterilization Cycles

In-Line Sterilization: Min. 25

Autoclaving: Min. 25

Technical References

Validation Guide:

SPK5768-e


Extractables Guide:

SPK5766-e


Order Codes

Cartridges	Pore Size [µm]	Pack Size [Pieces]	Test Pressure [bar psi]	Max. Diffusion [ml/min]	Min. Bubble Point [bar psi]
544250711	0.35 + 0.2	1	2.5 36	21	3.2 46
544250712	0.35 + 0.2	1	2.5 36	42	3.2 46
544250713	0.35 + 0.2	1	2.5 36	63	3.2 46

Chemically Defined Cell Culture Media

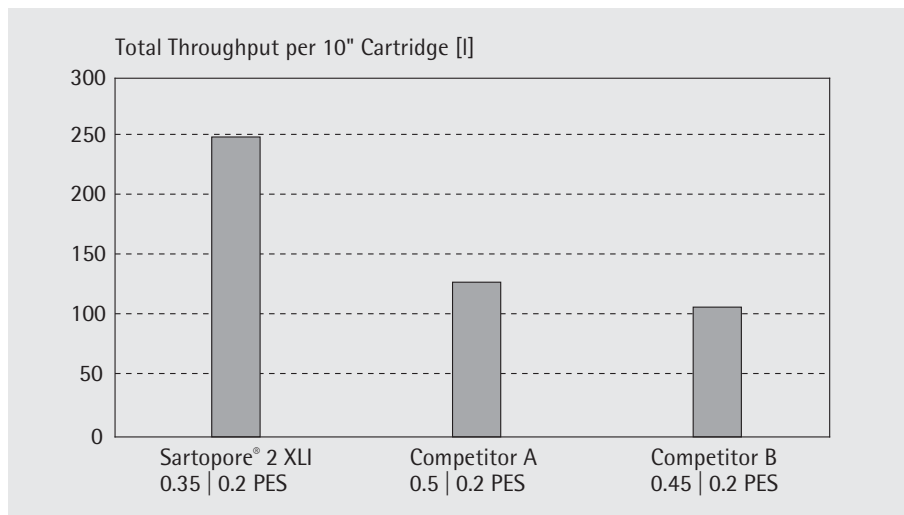

Ophthalmic Solution

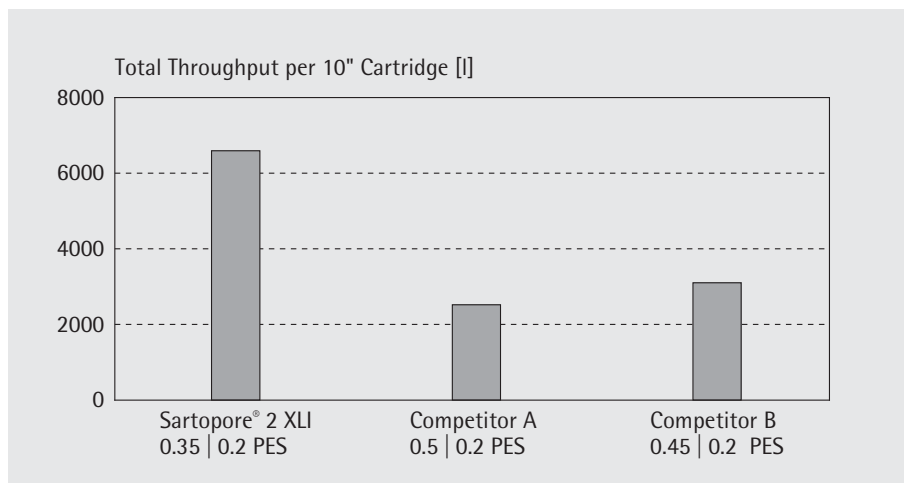

По вопросам продаж и поддержки обращайтесь:

Астана+7(7172)727-132, Волгоград(844)278-03-48, Воронеж(473)204-51-73, Екатеринбург(343)384-55-89,
 Казань(843)206-01-48, Краснодар(861)203-40-90, Красноярск(391)204-63-61, Москва(495)268-04-70,
 Нижний Новгород(831)429-08-12, Новосибирск(383)227-86-73, Ростов-на-Дону(863)308-18-15, Самара(846)206-03-16,
 Санкт-Петербург(812)309-46-40, Саратов(845)249-38-78, Уфа(347)229-48-12

sst@nt-rt.ru || sartorius.nt-rt.ru